



# Atrial Undersensing-Associated Premature Atrial Contractions: A Case Report

Oleksiy Skakun,<sup>1</sup> Yaroslava Vandzhura,<sup>2</sup> Ihor Vandzhura,<sup>2</sup> Khrystyna Symchych,<sup>3</sup> Anton Symchych<sup>4</sup>

## Abstract

Atrial undersensing is defined as the inability of the pacemaker to detect spontaneous atrial activity. A case of premature atrial contractions associated with atrial undersensing is presented. A 33-year-old woman presented with irregular heartbeat and general weakness. A single atrial stimulation (AAI) pacemaker was implanted seven years earlier for recurrent syncope associated with sinus arrest. Ambulatory ECG monitoring revealed multiple episodes of atrial undersensing resulting in premature atrial contractions (PACs). Occasionally, blocked PACs or PACs with aberrancy associated with atrial undersensing were seen. After improvement of atrial sensing, no episodes of undersensing were found and the complaints disappeared.

**Key words:** Artificial pacemaker; Atrial premature complexes; Heart block; Heart conduction systems.

1. Clinic of St Luka, Ivano-Frankivsk, Ukraine.
2. Ivano-Frankivsk National Medical University, Department of Internal Medicine #2 and Nursing, Ivano-Frankivsk, Ukraine.
3. Ivano-Frankivsk National Medical University, Department of Therapy, Family and Emergency Medicine Postgraduate Education, Ivano-Frankivsk, Ukraine.
4. Ivano-Frankivsk National Medical University, Department of General and Vascular Surgery, Ivano-Frankivsk, Ukraine.

### Citation:

Skakun O, Vandzhura Y, Vandzhura I, Symchych K, Symchych A. Atrial undersensing-associated premature atrial contractions: a case report. *Scr Med.* 2024 Jul-Aug;55(4):517-20.

### Corresponding author:

OLEKSIY SKAKUN  
E: olexiy109921@ukr.net  
T: +380968376087

Received: 6 May 2024

Revision received: 17 July 2024

Accepted: 17 July 2024


## Introduction

Undersensing is defined as the inability of the pacemaker to detect spontaneous myocardial depolarisation.<sup>1</sup> The prevalence of atrial undersensing ranges from 2.9 % to 20.7 % in patients with implanted pacemakers.<sup>2,3</sup> It's believed that atrial undersensing of < 10 % doesn't affect patients' functional ability and quality of life, whereas atrial undersensing of > 10 % is associated with a decrease in exercise tolerance and worse quality of life.<sup>4</sup> In addition, intermittent atrial undersensing in patients with VDD pacemakers is a possible mechanism of life-threatening ventricular arrhythmias.<sup>5</sup> Despite the large number of reported cases of undersensing, no association between undersensing and premature atrial or ventricular contraction has been reported.


A case of intermittent atrial undersensing in young patient with a single atrial stimulation (AAI) pacemaker resulting in premature atrial contractions (PACs) is described.

## Case history

A 33-year-old female patient presented to a doctor with complaints of irregular heartbeat and general weakness. These complaints occurred about 6 months ago and progressed gradually. Medical history: single atrial stimulation (AAI) pacemaker implanted seven years ago for recur-

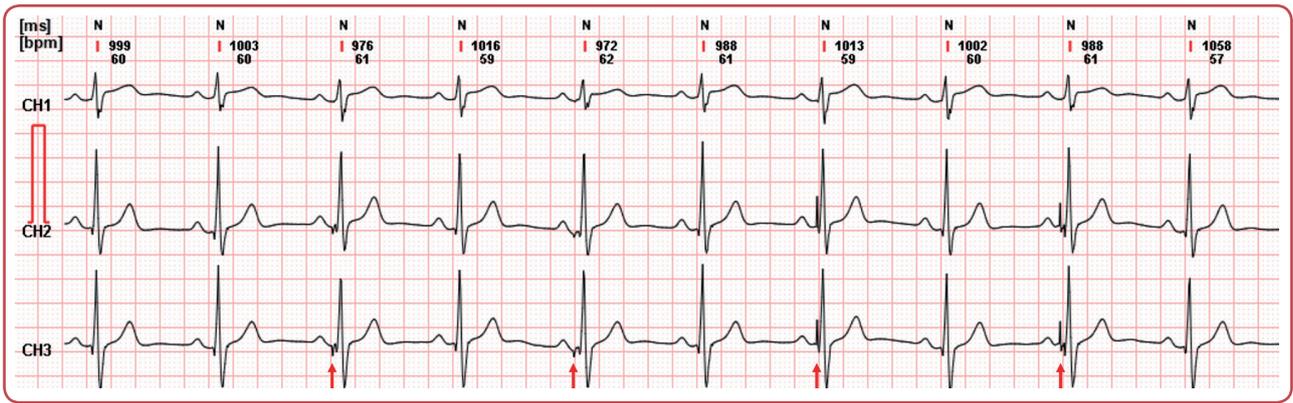

**Figure 1: Atrial undersensing**  
Pacing spikes (arrowed) are seen after P waves.

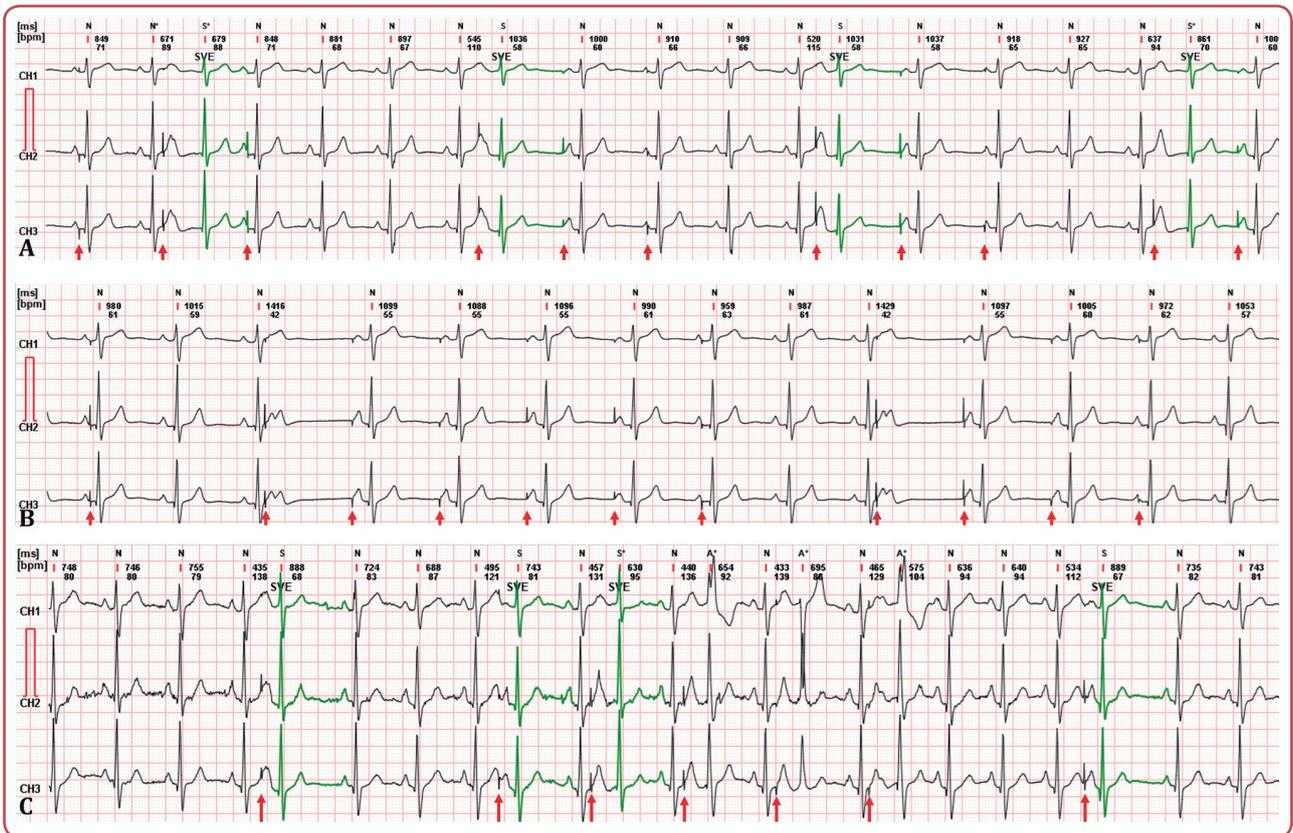

**Figure 2: Atrial undersensing: A) resulting in premature atrial contractions (PACs); B) resulting in blocked PACs; C) resulting in PACs with aberrancy**  
Pacing spikes are arrowed.

rent syncope associated with sinus arrest. Ambulatory electrocardiographic (ECG) monitoring was performed.

Ambulatory ECG monitoring revealed multiple episodes of undersensing (Figure 1), often resulting in premature atrial contractions (PACs) (Figure 2A). Occasionally, blocked PACs (Figure 2B) or PACs with aberrancy (Figure 2C) associated with atrial undersensing were seen. Eight thou-

sand two hundred twenty-one PACs (including 738 PACs with aberrancy) were detected. Each PAC was thought to be associated with atrial undersensing.

The patient was referred for the pacemaker check. The sensitivity of the atrial activity was increased (sensitivity threshold was decreased from 2.5 mV to 2.0 mV). Ambulatory ECG monitoring was performed after correction of atrial

sensing. Only 1 PAC (not related to undersensing) per day was found. In addition, complaints of irregular heartbeat and general weakness disappeared and there was a marked improvement in quality of life.

## Discussion

Presented patient was implanted AAI pacemaker due to a symptomatic episodes of sinus arrest. A DDD pacemaker with atrioventricular delay management is preferred for most patients, but young age may be a reason to avoid two leads and implant a single-chamber pacemaker.<sup>6</sup>

Atrial undersensing is one of the most common pacemaker malfunctions. It may be associated with irregular heartbeat due to PACs. In addition, PACs associated with atrial undersensing may be blocked (not conducted to the ventricles) or with aberrant conduction (right or left bundle branch block). The response of the atria and ventricles to atrial pacing in atrial undersensing depends on the timing of the atrial pacing spike. If the atrial pacing spike occurs very early after the P wave (before, during or just after the QRS complex), atrial depolarisation (and the P wave) doesn't occur due to the refractory period in the atria. If the atrial pacing spike appears when the atria come out of their refractory period but during the refractory period of the atrioventricular node, the ECG shows a P wave without a QRS complex (blocked PAC). If the atrial pacing spike occurs later, a P wave followed by a QRS complex is seen. If the impulse spread to the ventricles during the refractory period in the one of the bundle branches, aberrantly conducted PAC is seen.

Atrial undersensing should be suspected in any patient with an implanted pacemaker (with an atrial lead) and PACs, as the pacing spike is sometimes poorly visible. Correction of atrial sensing is essential for patients with this condition.

## Conclusion

Atrial undersensing may result in symptomatic PACs. Improvement of atrial sensing may completely eliminate atrial undersensing and the patients' symptoms.

## Ethics

Our institution does not require ethics approval for reporting individual cases or case series. A written informed consent for anonymised patient information to be published has been obtained from the patient.

## Acknowledgement

We extend our gratitude to the patient and the entire medical team providing care.

## Conflicts of interest

The authors declare that there is no conflict of interest.

## Funding

This research received no specific grant from any funding agency in the public, commercial, or not-for-profit sectors.

## Data access

The data that support the findings of this study are available from the corresponding author upon reasonable individual request.

## Author ORCID numbers

Oleksii Skakun (OS):  
0000-0003-4745-9858  
Yaroslava Vandzhura (YV):  
0000-0003-2525-371X  
Ihor Vandzhura (IV):  
0000-0001-5905-487X  
Khrystyna Symchych (KS):  
0000-0002-6519-8500  
Anton Symchych (AS):  
0000-0002-4547-9938

## Author contributions

Conceptualisation: OS, YV, IV  
Methodology: OS, YV  
Software: OS, KS, AS  
Validation: VY, KS  
Formal analysis: VI, AS  
Investigation: OS  
Resources: OS, YV  
Data curation: YV, IV  
Writing - original draft: OS, YV, IV  
Writing - review and editing: SK, AS  
Visualisation: OS, IV  
Supervision: OS  
Project administration: OS.

## References

1. Safavi-Naeini P, Saeed M. Pacemaker troubleshooting: common clinical scenarios. *Tex Heart Inst J.* 2016 Oct 1;43(5):415-8. doi: 10.14503/THIJ-16-5918.
2. Antonioli GE, Ansani L, Barbieri D, Guardigli G, Perco-co GF, Toselli T. Italian multicenter study on a single lead VDD pacing system using a narrow atrial dipole spacing. *Pacing Clin Electrophysiol.* 1992 Nov;15(11 Pt 2):1890-3. doi: 10.1111/j.1540-8159.1992.tb02988.x.
3. Wiegand UK, Bode F, Schneider R, Brandes A, Haase H, Katus HA, et al. Diagnosis of atrial undersensing in dual chamber pacemakers: impact of autodiagnostic features. *Pacing Clin Electrophysiol.* 1999 Jun;22(6 Pt 1):894-902. doi: 10.1111/j.1540-8159.1999.tb06813.x.
4. Van Campen CM, De Cock CC, Huijgens J, Visser CA. Clinical relevance of loss of atrial sensing in patients with single lead VDD pacemakers. *Pacing Clin Electrophysiol.* 2001 May;24(5):806-9. doi: 10.1046/j.1460-9592.2001.00806.x.
5. Palanca V, Navarro A, Jiménez J, Quesada A, Morell S, Roda J. Intermittent atrial undersensing in single-lead VDD pacemakers in patients with bradycardia-sensitive repolarisation: a possible mechanism for ventricular arrhythmia. *Rev Esp Cardiol.* 2010 Feb 1;63(2):229-32. doi: 10.1016/S1885-5857(10)70042-6.
6. Glikson M, Nielsen JC, Kronborg MB, Michowitz Y, Auticcho A, Barbash IM, et al. 2021 ESC Guidelines on cardiac pacing and cardiac resynchronisation therapy: Developed by the Task Force on cardiac pacing and cardiac resynchronisation therapy of the European Society of Cardiology (ESC) With the special contribution of the European Heart Rhythm Association (EHRA). *Eur Heart J.* 2021; 42(35):3427-520. doi:10.1093/eurheartj/ehab364.